




VAMP © Vascular Access Monitoring & Surveillance Flow Chart

Submitted by: Lawrence Spergel, MD, FACS
Dialysis Management Medical Group
San Francisco, CA USA

This educational item was produced through the AV Fistula First Breakthrough Initiative Coalition, sponsored by the Centers for Medicare and Medicaid Services (CMS), Department of Health and Human Services (DHHS). The content of this publication does not necessarily reflect the views or policies of the DHHS, nor does mention of trade names, commercial products, or organizations imply endorsement by the U.S. Government. The author(s) assume full responsibility for the accuracy and completeness of the ideas presented, and welcome any comments and experiences with this product.

VAMP © Vascular Access Monitoring & Surveillance Flow Chart

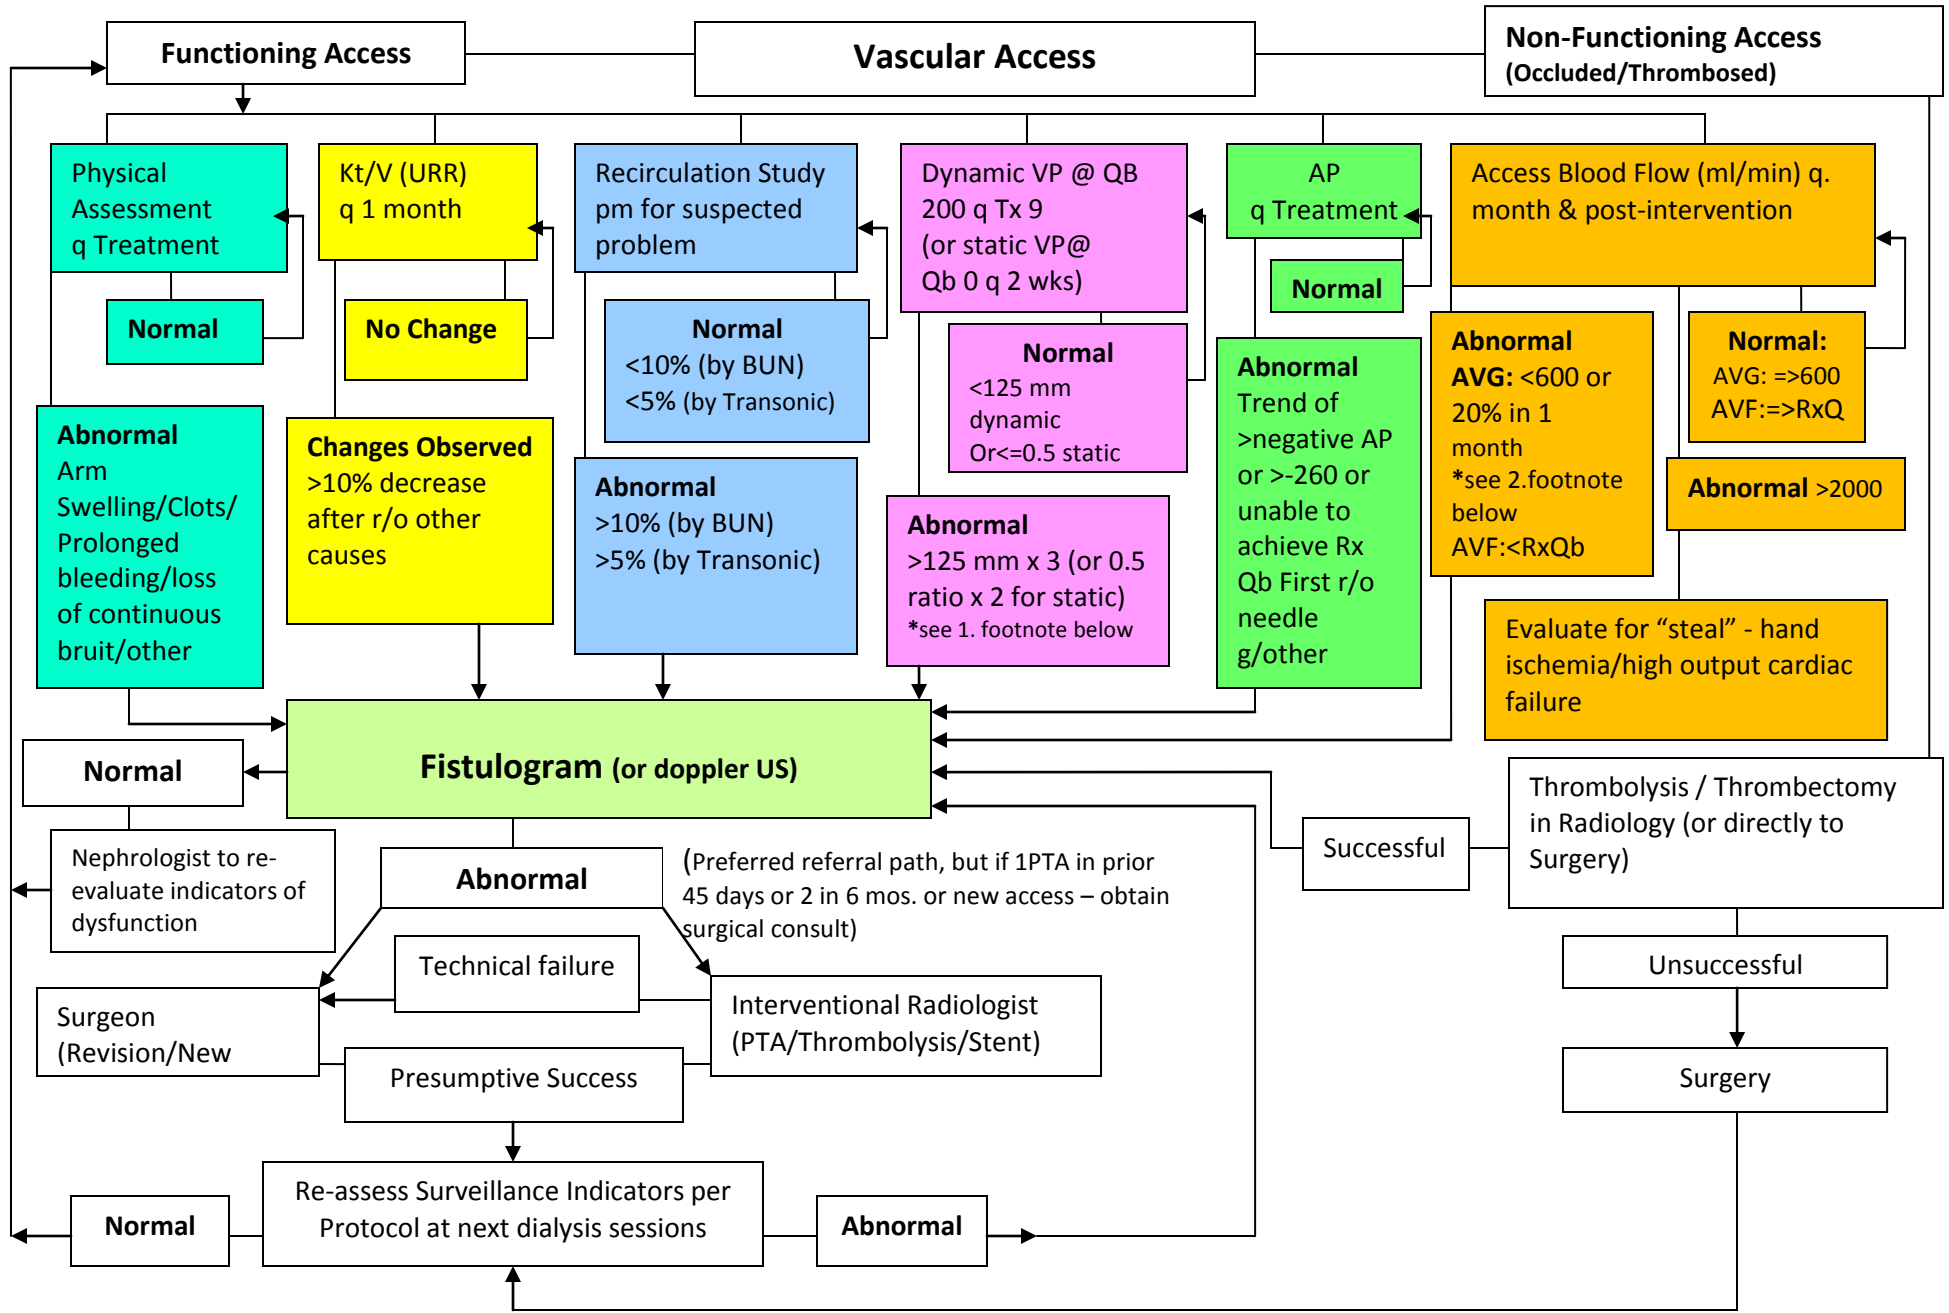

1. For static pressures, see attached protocol for measuring both venous and arterial intra-access pressure ratios.

2. If AVG access blood flow falls by 20% in 1 month, and flow is below 1000, repeat next session and if still lower by 20%, refer for fistulogram.